

1 **Supplementary Material**

2 **For**

3 **A Novel Methodology for Assessing the Hygroscopicity of Aerosol Filter Samples**

4 **Nagendra Raparathi¹, Anthony S. Wexler^{1,2,3,4}, Ann M. Dillner¹**

5 ¹Air Quality Research Center, University of California, Davis, 95616 CA, USA

6 ²Mechanical and Aerospace Engineering, University of California, Davis, 95616 CA, USA

7 ³Civil and Environmental Engineering, University of California, Davis, 95616 CA, USA


8 ⁴Land, Air, and Water Resources, University of California, Davis, 95616 CA, USA

9
10 *Correspondence to:* Ann M. Dillner (amdillner@ucdavis.edu)


31 **Table S1.** Air density and mass obtained for room and measured relative humidities (RHs) from
 32 Psychrometric Chart

	1st Day	2nd day	3rd day	4th day	5th day
T (°C) - <i>Observed</i>	20.5	21.2	20.3	19.7	19.5
RH (%) - <i>Observed</i>	41.4	63.9	52.4	37.2	49.8
P (mm Hg) - <i>Observed</i>	767.6	764.3	762.5	767.8	764.5
<i>From Online Psychrometric Chart</i>	Specific volume (m³/kg)				
Room	0.832	0.843	0.839	0.828	0.833
84.3%	0.840	0.847	0.845	0.837	0.840
90.8%	0.842	0.848	0.847	0.838	0.841
97.5%	0.843	0.850	0.848	0.840	0.842
<i>Inverse of specific volume</i>	Air density (kg/m³)				
Room	1.202	1.186	1.192	1.207	1.200
84.3%	1.190	1.181	1.183	1.195	1.190
90.8%	1.188	1.179	1.181	1.193	1.189
97.5%	1.186	1.176	1.179	1.190	1.188
<i>Mass (in µg)</i>	Change in the mass (µg) of air from measured RHs to room RH				
	1st Day	2nd day	3rd day	4th day	5th day
84.3%	233	114	172	264	204
90.8%	245	120	193	247	196
97.5%	293	183	237	323	240



33

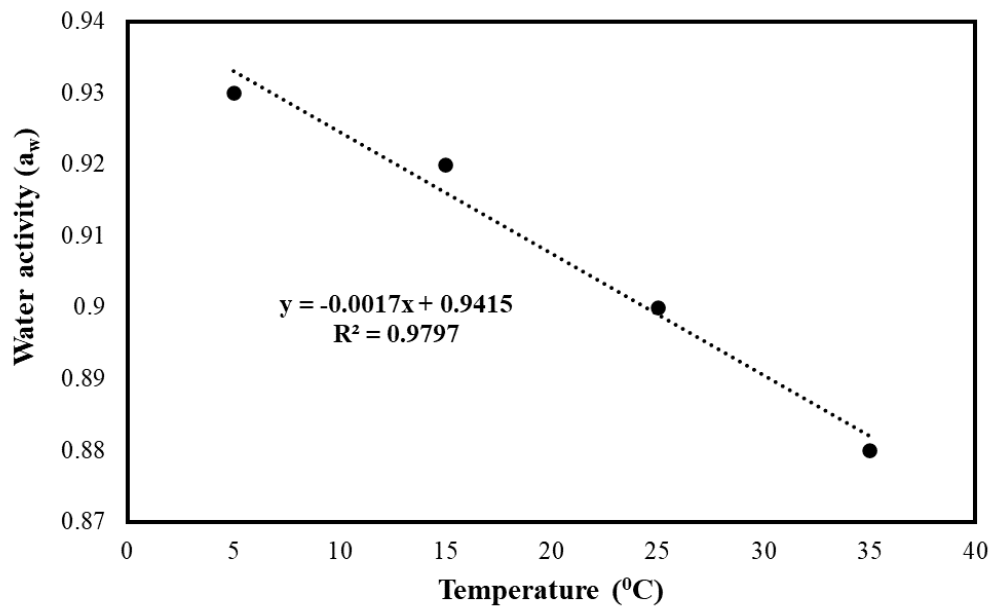

34
 35 **Figure S1.** Water activity of saturate $BaCl_2 \cdot 2H_2O$ at different temperatures (Source: Wang et al.,
 36 2012)

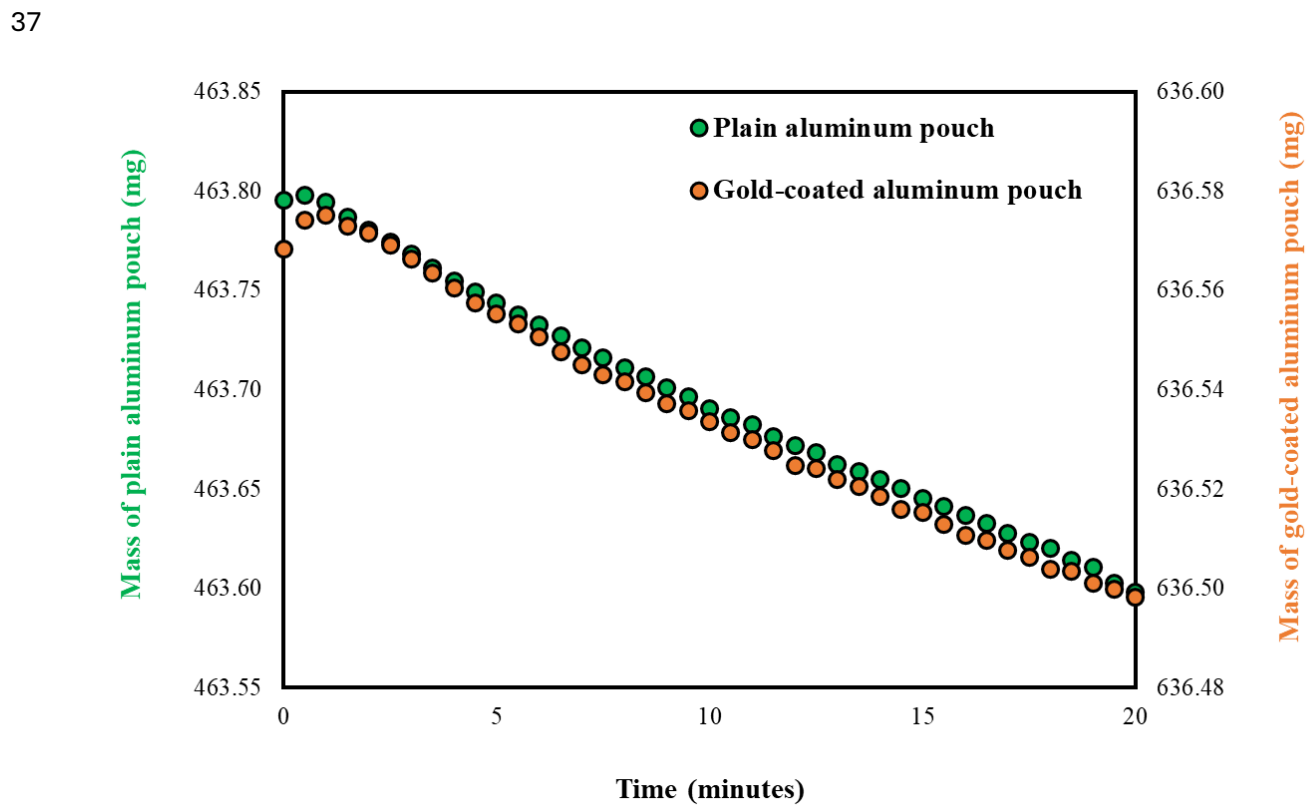


38
 39 **Figure S2.** Comparison of the variation in wet weight of plain and gold-coated aluminum
 40 pouches with loaded filters

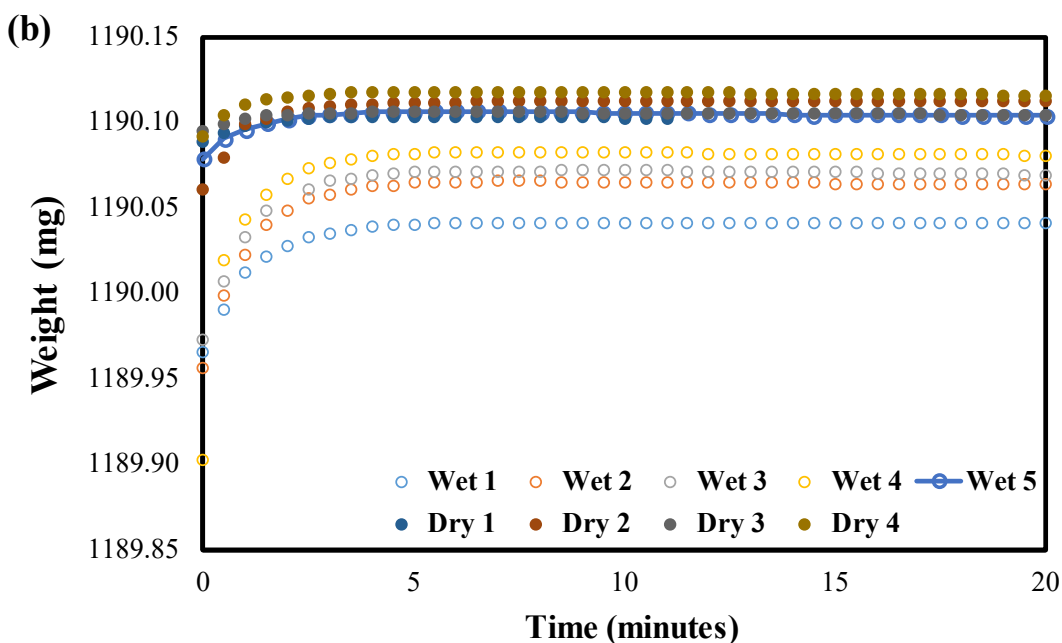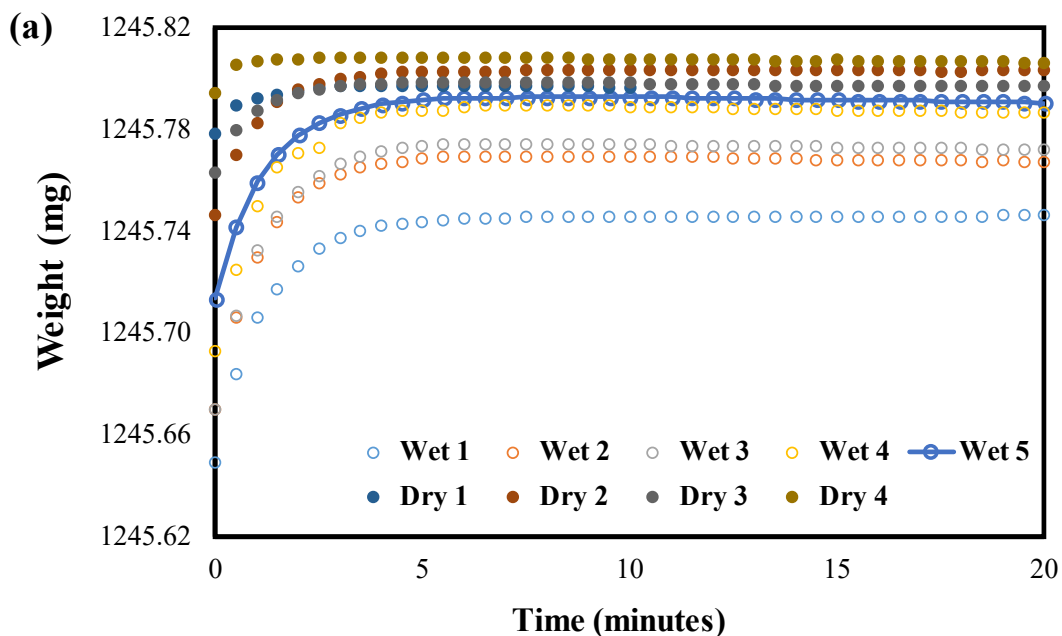

41
 42 **Figure S3.** Variation in the weight of the plain aluminum pouch with a Teflon filter (a) 84.3%
 43 and (b) 90.5% over time starting when the pouch is removed from the respective chamber and
 44 placed on the balance. Hollow circles represent the transfer from the wet chamber to the balance,
 45 while solid circles depict the transfer from the dry desiccator to the balance


46
 47

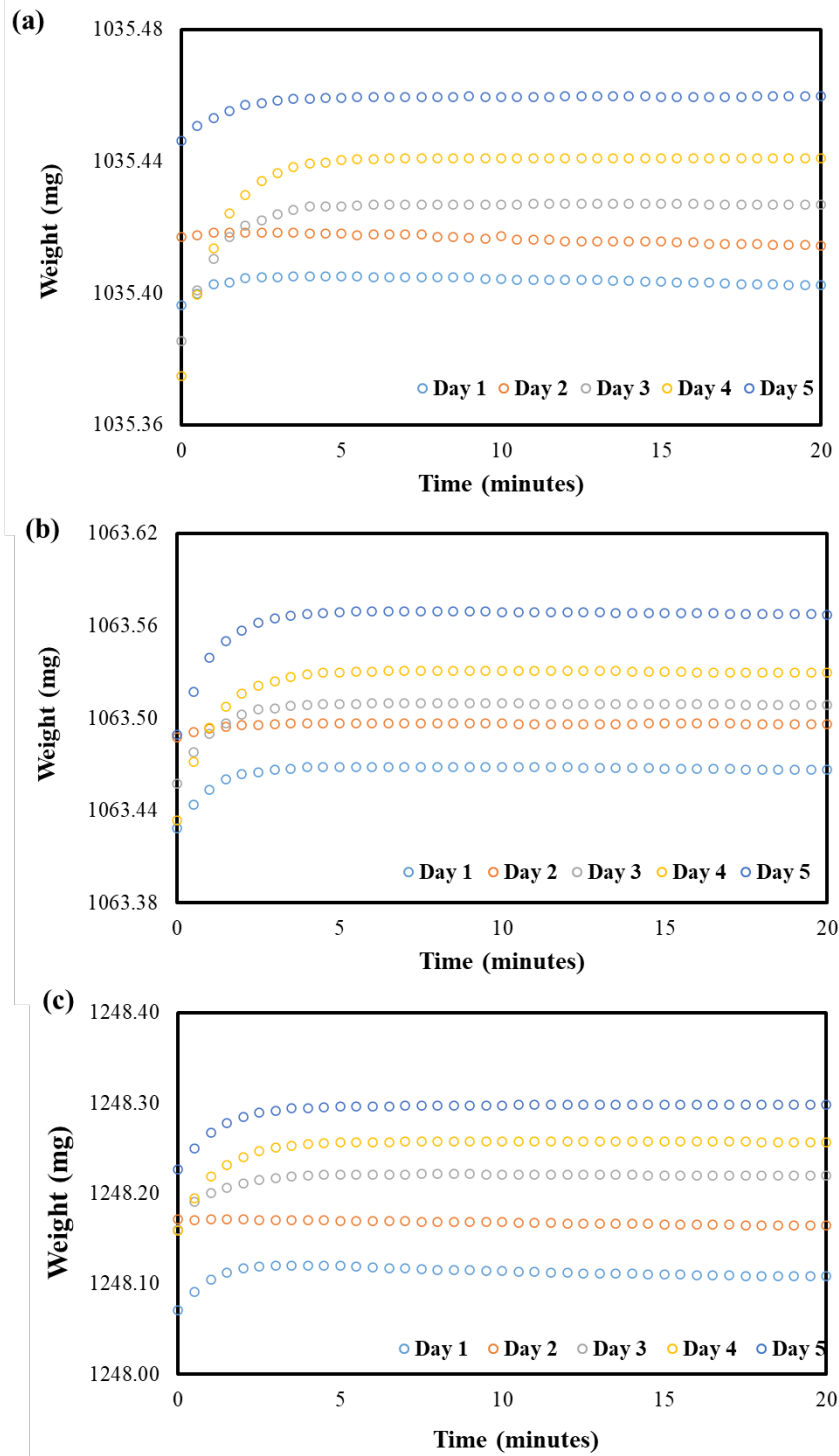

48

49 **Figure S4.** Variation in the wet weight of the plain aluminum pouch without a Teflon filter (a)
 50 84.3%, (b) 90.8% and (c) 97.5% over time starting when the pouch is removed from the
 51 respective chamber and placed on the balance.

52

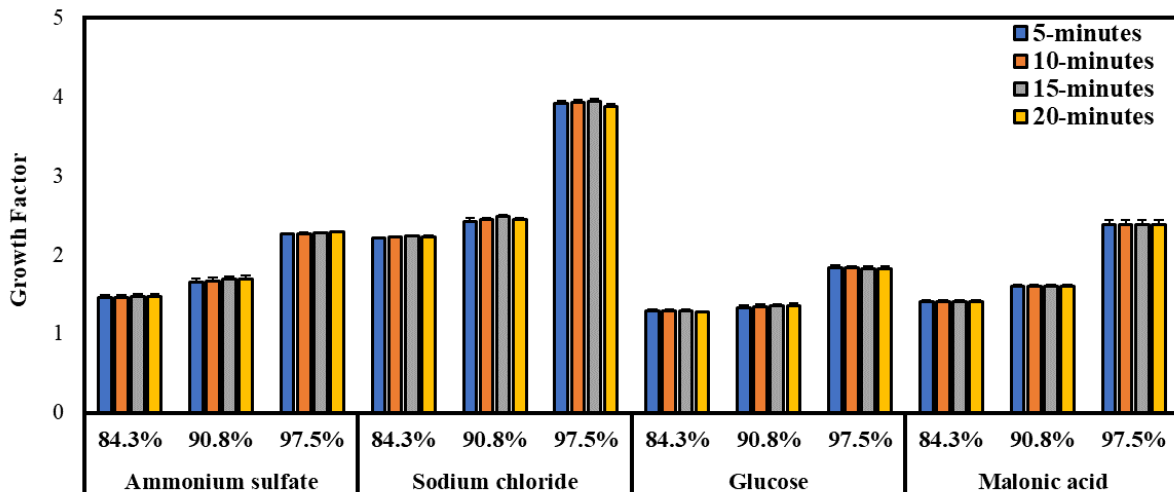

53

54 **Figure S5.** Comparison of estimated GFs from the 20 minutes wet weighing interval with the 5,
 55 10, and 15-minute intervals. Error bar represents the standard deviation.

56

57